


Figure 1

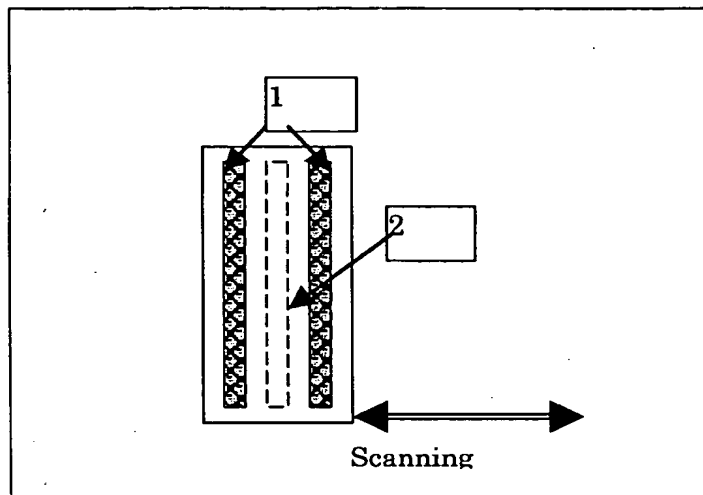

Device viewed from the irradiated tissue side

Figure 2

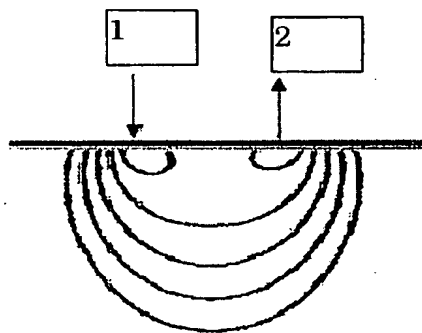


Figure 3

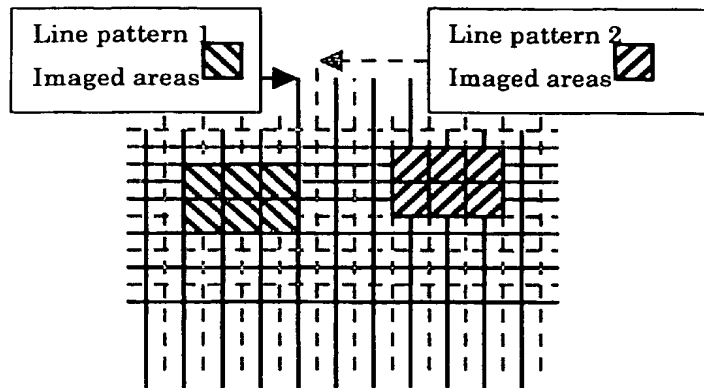


Figure 4

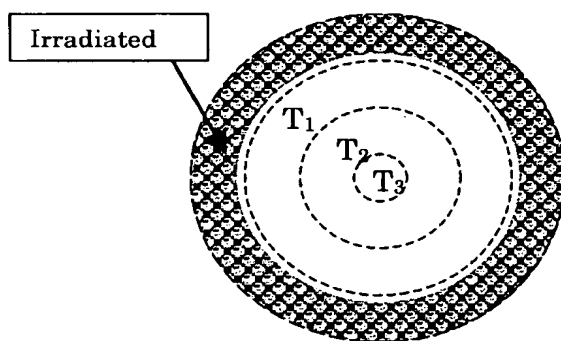


Figure 5

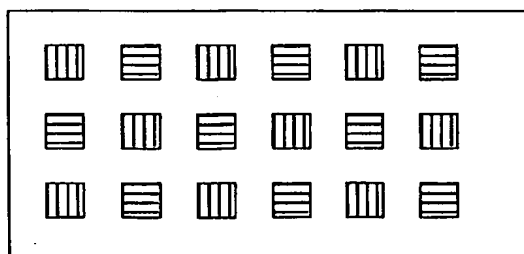


Figure 6

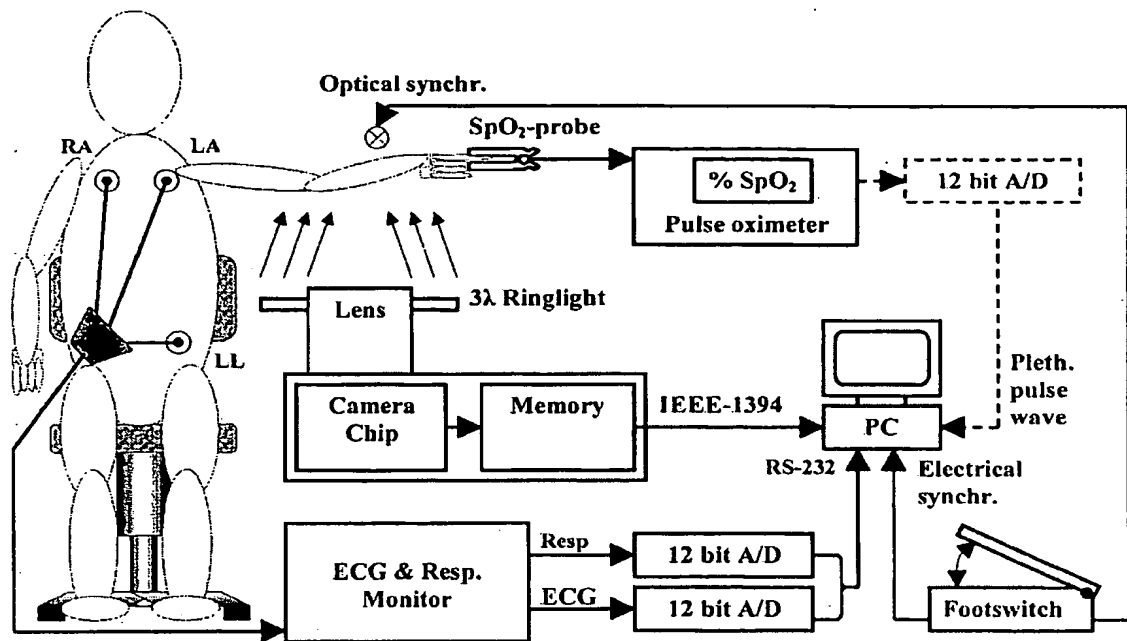


Figure 7

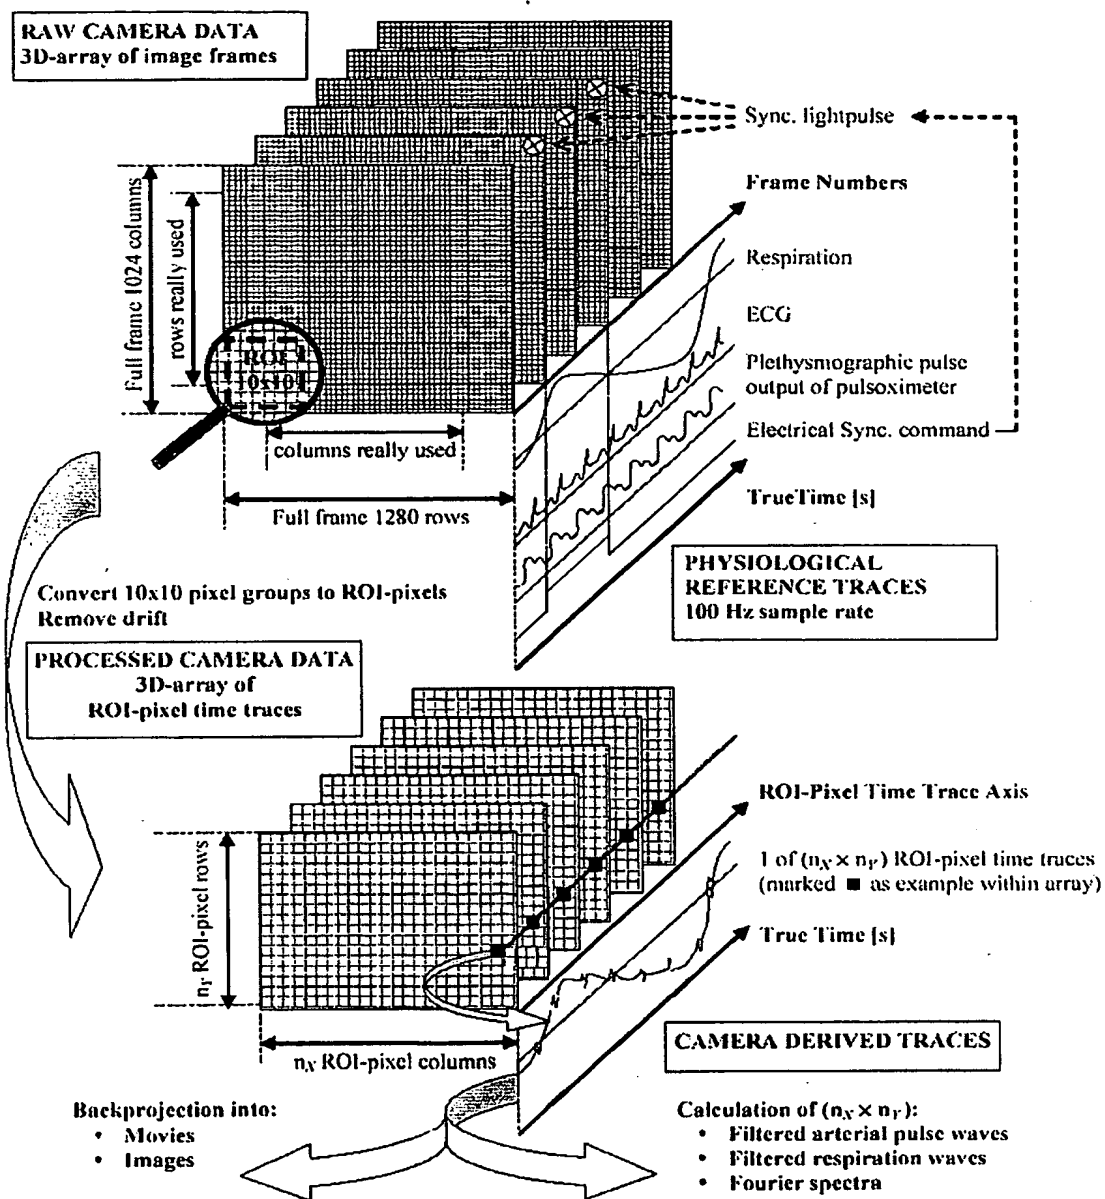


Figure 8

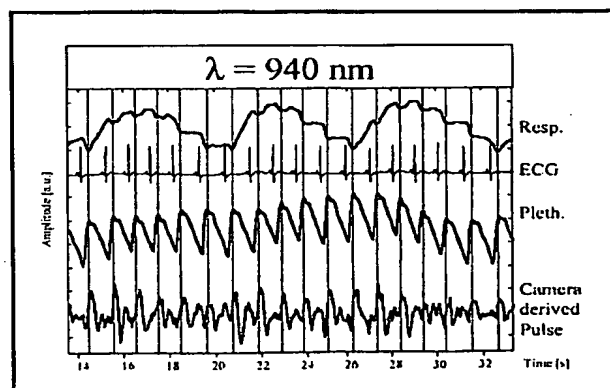
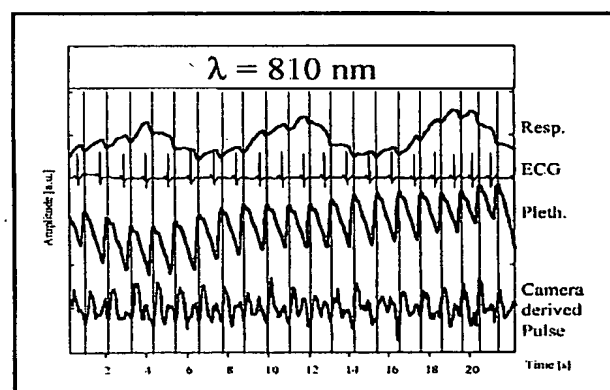
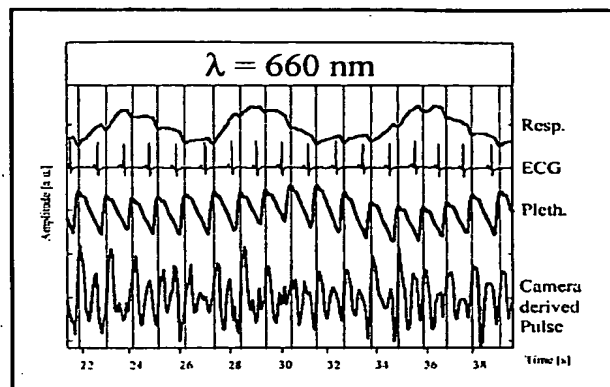


Figure 9

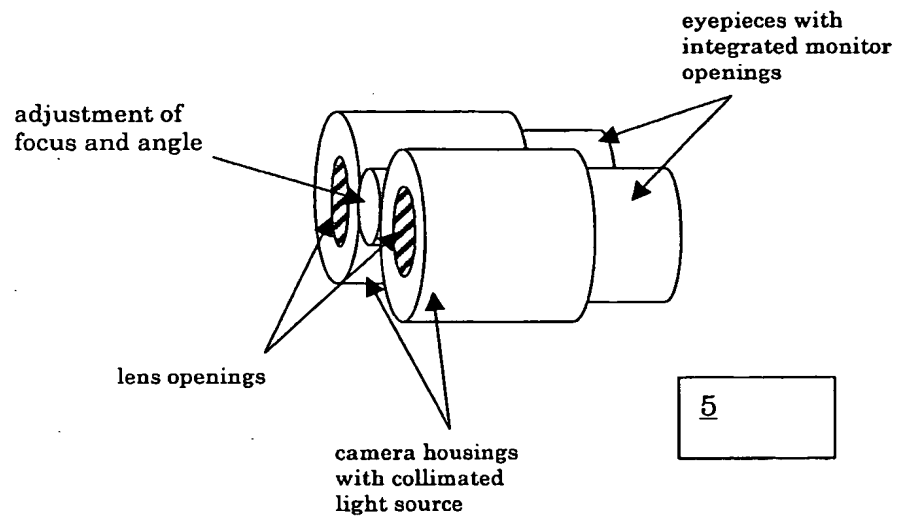


Figure 10

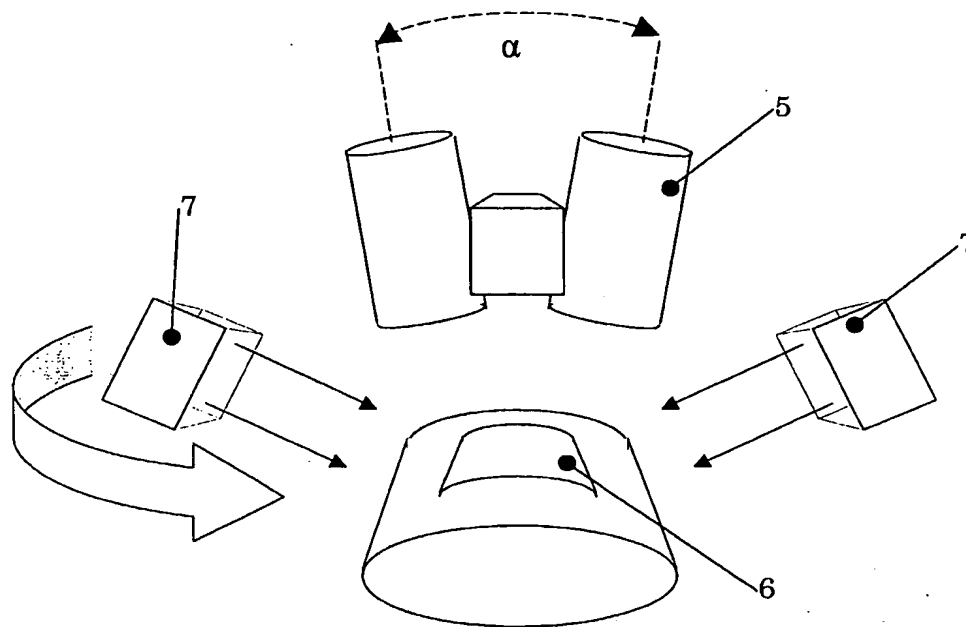


Figure 11

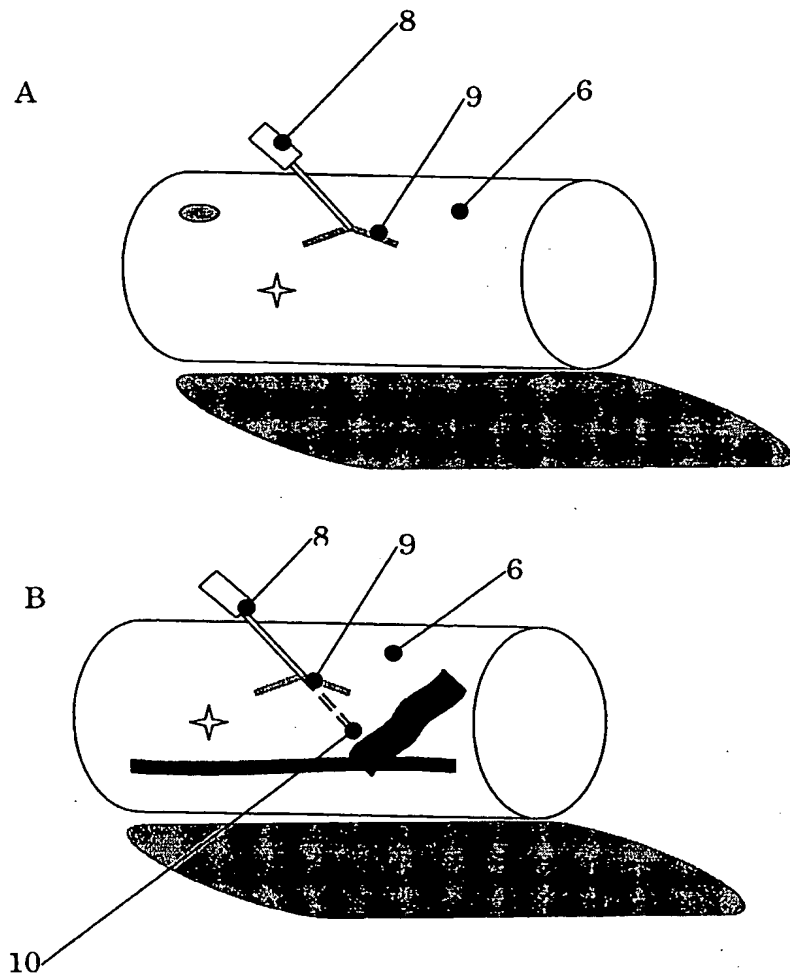




Figure 16



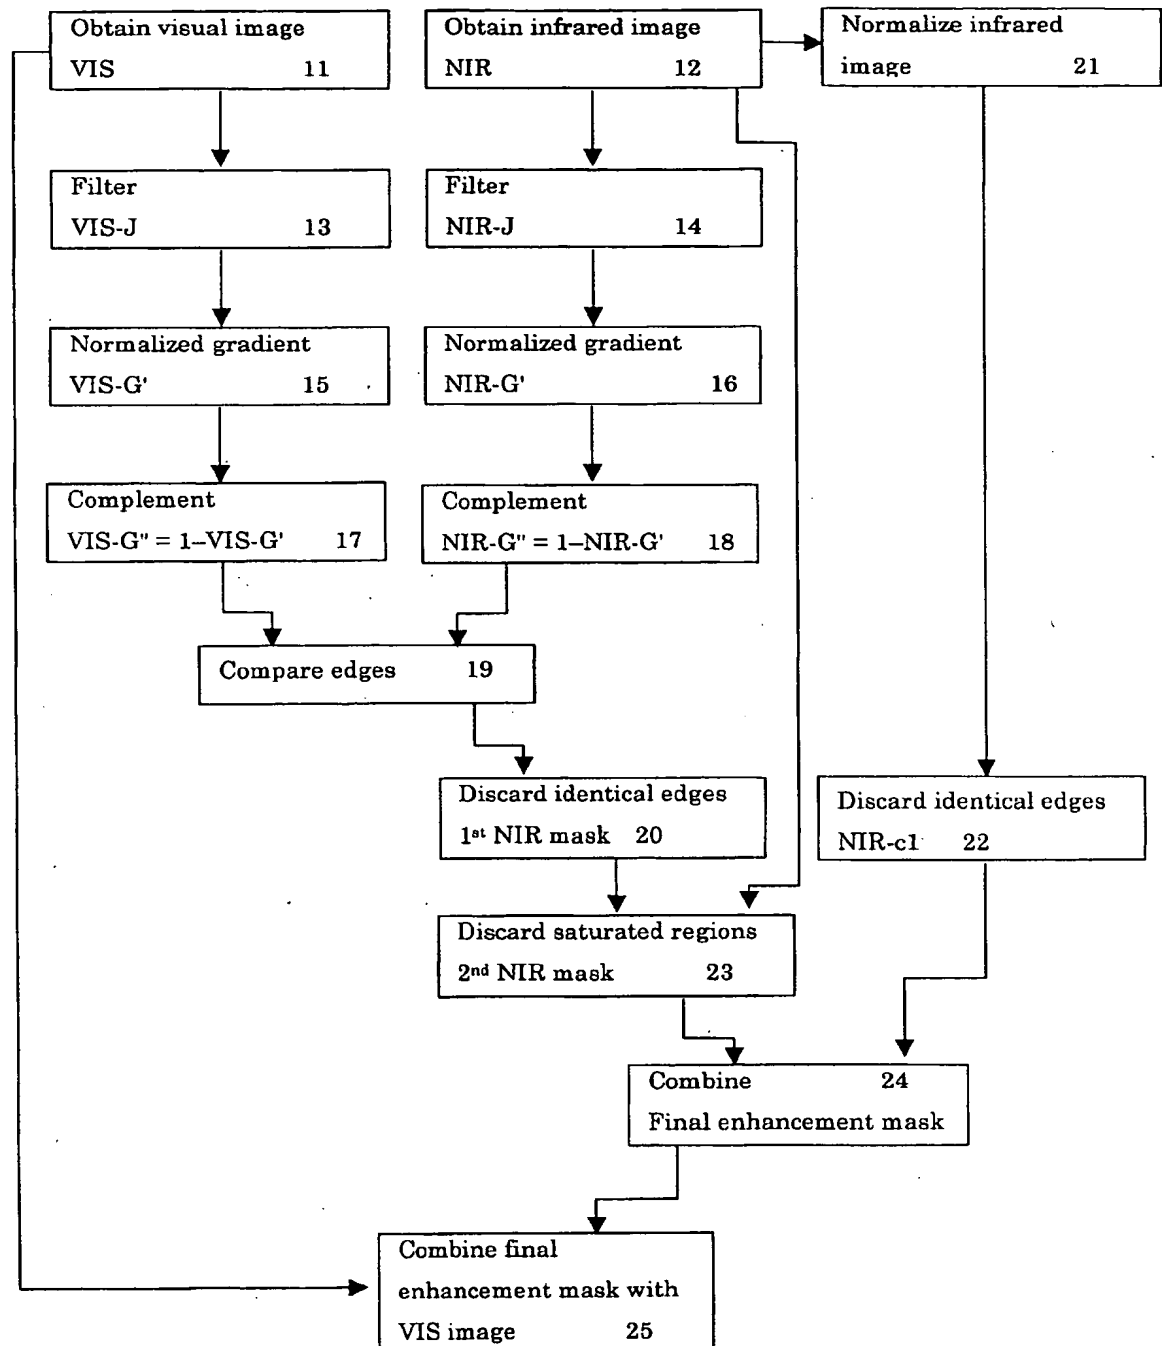



Figure 13

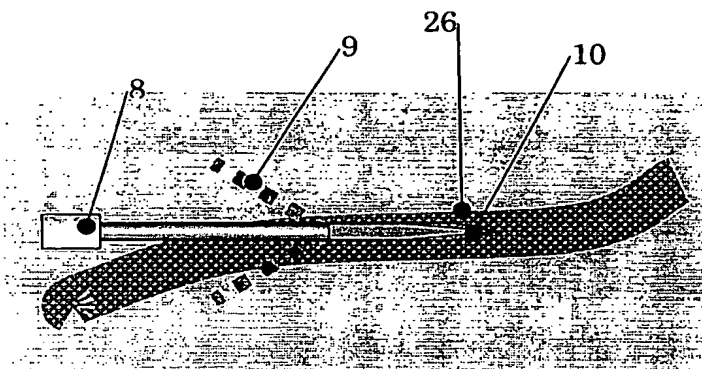

A

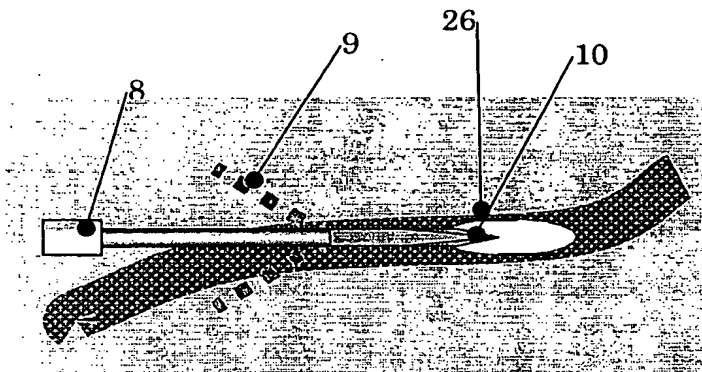

B

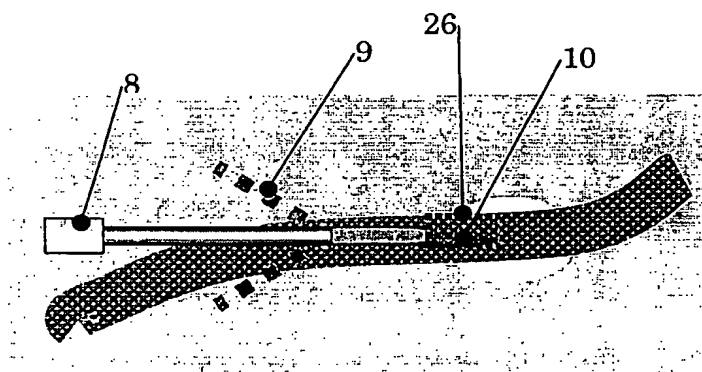

C